

# R&S® ZNLE VECTOR NETWORK ANALYZER

## Specifications



Data Sheet  
Version 04.00

# CONTENTS

<b>Definitions .....</b>	<b>3</b>
<b>Specifications.....</b>	<b>4</b>
Measurement range .....	4
Measurement speed.....	5
Measurement accuracy .....	6
Effective system data.....	7
Factory-calibrated system data.....	7
Test port output .....	8
Test port input .....	9
Additional front panel connectors.....	10
Display .....	10
Rear panel connectors.....	10
<b>Options .....</b>	<b>11</b>
R&S®FPL1-B10 .....	11
<b>General data .....</b>	<b>12</b>
<b>Dimensions (in mm).....</b>	<b>13</b>
<b>Ordering information .....</b>	<b>14</b>

# Definitions


## General

Product data applies under the following conditions:

- Three hours storage at ambient temperature followed by 30 minutes warm-up operation
- Specified environmental conditions met
- Recommended calibration interval adhered to
- All internal automatic adjustments performed, if applicable

## Specifications with limits

Represent warranted product performance by means of a range of values for the specified parameter. These specifications are marked with limiting symbols such as  $<$ ,  $\leq$ ,  $>$ ,  $\geq$ ,  $\pm$ , or descriptions such as maximum, limit of, minimum. Compliance is ensured by testing or is derived from the design. Test limits are narrowed by guard bands to take into account measurement uncertainties, drift and aging, if applicable.

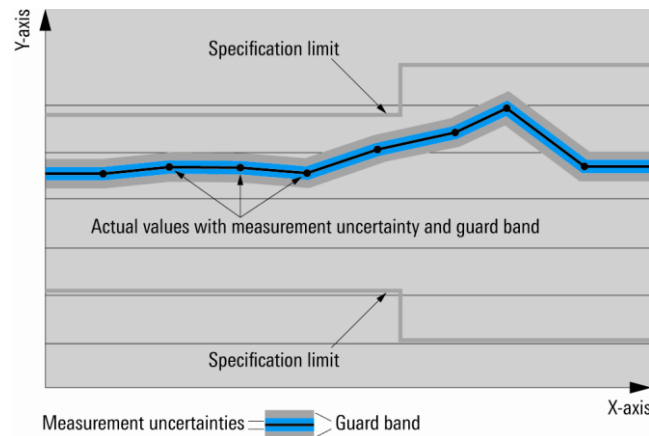

## Specifications without limits

Represent warranted product performance for the specified parameter. These specifications are not specially marked and represent values with no or negligible deviations from the given value (e.g. dimensions or resolution of a setting parameter). Compliance is ensured by design.

## Typical data (typ.)

Characterizes product performance by means of representative information for the given parameter. When marked with  $<$ ,  $>$  or as a range, it represents the performance met by approximately 80 % of the instruments at production time. Otherwise, it represents the mean value.

## Nominal values (nom.)

Characterize product performance by means of a representative value for the given parameter (e.g. nominal impedance). In contrast to typical data, a statistical evaluation does not take place and the parameter is not tested during production.

## Measured values (meas.)

Characterize expected product performance by means of measurement results gained from individual samples.

## Uncertainties

Represent limits of measurement uncertainty for a given measurand. Uncertainty is defined with a coverage factor of 2 and has been calculated in line with the rules of the Guide to the Expression of Uncertainty in Measurement (GUM), taking into account environmental conditions, aging, wear and tear.

Device settings and GUI parameters are indicated as follows: "parameter: value".

Typical data as well as nominal and measured values are not warranted by Rohde & Schwarz.

# Specifications



## Measurement range

Impedance		50 $\Omega$
Test port connector		N female
Number of test ports		2
Frequency range <sup>1</sup>	without R&S <sup>®</sup> ZNLE-B100 low frequency extension option	
	R&S <sup>®</sup> ZNLE3	1 MHz to 3 GHz
	R&S <sup>®</sup> ZNLE4	1 MHz to 4.5 GHz
	R&S <sup>®</sup> ZNLE6	1 MHz to 6 GHz
	with R&S <sup>®</sup> ZNLE-B100 B100 low frequency extension option	
	R&S <sup>®</sup> ZNLE3	100 kHz to 3 GHz
	R&S <sup>®</sup> ZNLE4	100 kHz to 4.5 GHz
R&S <sup>®</sup> ZNLE6	100 kHz to 6 GHz	

Static frequency accuracy		(time since last adjustment $\times$ aging rate) + temperature drift + calibration accuracy
Aging per year		$\pm 1 \times 10^{-6}$
Temperature drift (+5 °C to +40 °C)		$\pm 1 \times 10^{-6}$
Achievable initial calibration accuracy		$\pm 5 \times 10^{-7}$

Frequency resolution		1 Hz
Number of measurement points	per trace	1 to 5001
Measurement bandwidth	1/1.5/2/3/5/7 steps	1 Hz to 500 kHz

		<b>specification</b>	<b>typical</b>
Dynamic range <sup>1,2</sup>	100 kHz to 50 MHz	> 100 dB	110 dB
	50 MHz to 6 GHz	> 110 dB	120 dB

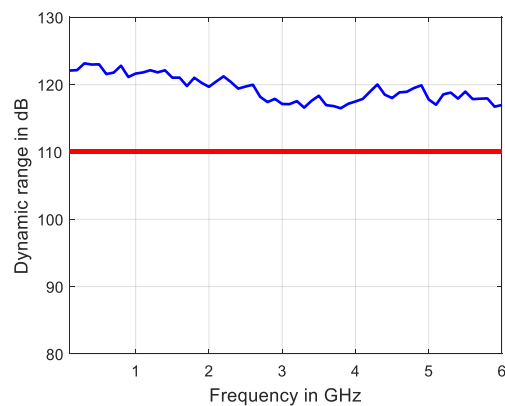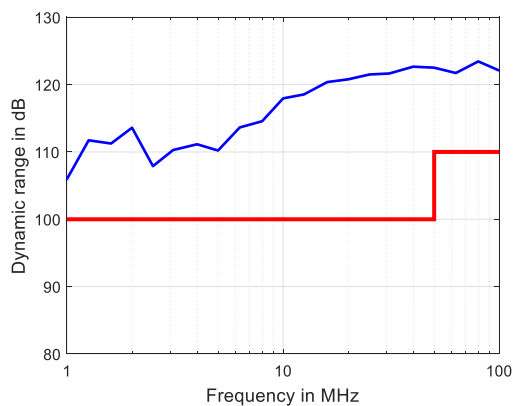

*Dynamic range in dB versus frequency for the R&S<sup>®</sup>ZNLE*


<sup>1</sup> Specified and typical data given in this data sheet apply to the R&S<sup>®</sup>ZNLE3, the R&S<sup>®</sup>ZNLE4 and the R&S<sup>®</sup>ZNLE6; please note their respective frequency ranges.

<sup>2</sup> The dynamic range is defined as the difference between 0 dBm source power and the RMS value of the data trace of the transmission magnitude, which is produced by noise and crosstalk with the test ports short-circuited. The specification applies at 10 Hz measurement bandwidth, without system error correction. The dynamic range can be increased by using a measurement bandwidth of 1 Hz.

## Measurement speed

Measured with firmware version 1.00 and Windows 10, 64 bit.

Measurement time	for 201 measurements points, with 200 MHz span, 500 kHz measurement bandwidth	$T_{\text{SWEEP}}$	$T_{\text{CYCLE}}$	
	with 900 MHz center frequency	< 4.0 ms	< 5.0 ms	
Acquisition time per point ( $T_{\text{ACQ}}$ )	500 kHz measurement bandwidth, CW mode	< 10 $\mu\text{s}$		
Sampling time per point ( $T_{\text{SAMPLE}}$ )	at 500 kHz measurement bandwidth	4.5 $\mu\text{s}$		
Time for measurement and data transfer	for 201 measurements points, with 800 MHz start frequency, 1 GHz stop frequency, 500 kHz measurement bandwidth <sup>3</sup>	IEC/IEEE	VXI11	HiSLIP
		over 1 Gbit/s LAN		
		10 ms typ.	10 ms typ.	10 ms typ.
Data transfer time	for 201 measurements points (magnitude)	3 ms typ.	2.5 ms typ.	2.5 ms typ.
Switching time between channels	with a maximum of 2001 points	< 5 ms		
Switching time between two preloaded instrument settings	with a maximum of 2001 points	< 5 ms		

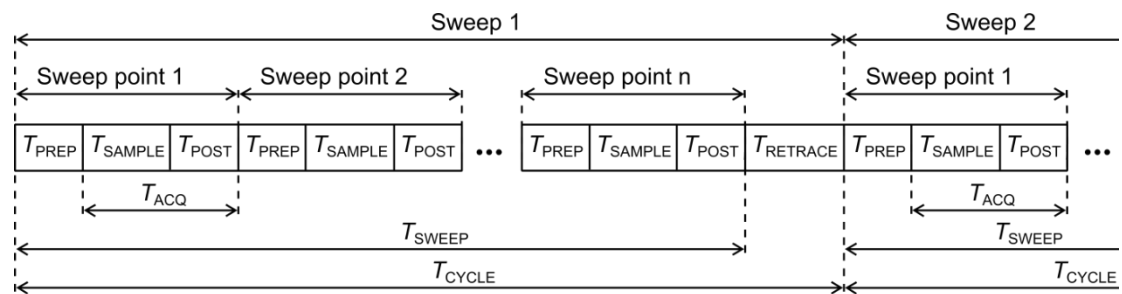

- $T_{\text{PREP}}$  Preparation time required to set up the internal hardware components
- $T_{\text{SAMPLE}}$  Sampling time (approximately equal to the settling time of the digital filters)
- $T_{\text{POST}}$  Time required for hardware postprocessing
- $T_{\text{ACQ}}$  Acquisition time ( $T_{\text{SAMPLE}} + T_{\text{POST}}$ )
- $T_{\text{SWEEP}}$  Time required for one sweep
- $T_{\text{RETRACE}}$  Time between two sweeps
- $T_{\text{CYCLE}}$  Sweep cycle time ( $T_{\text{SWEEP}} + T_{\text{RETRACE}}$ )

### Measurement sequence

Typical sweep times versus number of measurement points <sup>1, 4</sup>					
Number of measurement points	51	201	401	1601	5001
800 MHz start frequency, 1 GHz stop frequency, 100 kHz measurement bandwidth					
With correction switched off	2.4 ms	4.9 ms	8.7 ms	31.2 ms	94 ms
With 2-port TOSM calibration	3.9 ms	9.6 ms	16.7 ms	61.7 ms	189 ms
800 MHz start frequency, 1 GHz stop frequency, 1 kHz measurement bandwidth					
With correction switched off	66 ms	258 ms	515 ms	2055 ms	6400 ms
With 2-port TOSM calibration	132 ms	515 ms	1028 ms	4100 ms	12780 ms
100 MHz start frequency, 3 GHz stop frequency, 100 kHz measurement bandwidth					
With correction switched off	3.9 ms	9.1 ms	14.5 ms	36.7 ms	102 ms
With 2-port TOSM calibration	7.3 ms	17.7 ms	28.8 ms	73.3 ms	206 ms
100 MHz start frequency, 3 GHz stop frequency, 1 kHz measurement bandwidth					
With correction switched off	68 ms	262 ms	519 ms	2055 ms	6390 ms
With 2-port TOSM calibration	136 ms	524 ms	1040 ms	4110 ms	12800 ms
100 MHz start frequency, 6 GHz stop frequency, 100 kHz measurement bandwidth					
With correction switched off	3.9 ms	9.5 ms	15.4 ms	47 ms	104 ms
With 2-port TOSM calibration	7.3 ms	18.8 ms	30.5 ms	95 ms	209 ms
100 MHz start frequency, 6 GHz stop frequency, 1 kHz measurement bandwidth					
With correction switched off	68 ms	263 ms	521 ms	2070 ms	6400 ms
With 2-port TOSM calibration	136 ms	525 ms	1042 ms	4120 ms	12800 ms


<sup>3</sup> In continuous mode, no additional time for data transfer is needed as this occurs simultaneously during the measurement.

<sup>4</sup> Sweep time is to be understood as cycle time; static frequency accuracy of the instrument applies; measured with firmware version 1.00, Windows 10.

## Measurement accuracy


This data is valid between +18 °C and +28 °C, provided the temperature has not varied by more than 1 °C since calibration. Validity of the data is conditional on the use of an R&S®ZV-Z270 calibration kit and TOSM/SOLT calibration. This calibration kit is used to achieve the effective system data specified below. Frequency points, measurement bandwidth and sweep time have to be identical for measurement and calibration (no interpolation allowed).

Accuracy of transmission measurements		
Above 100 kHz	+5 dB to -35 dB	< 0.05 dB or < 0.5°
	-35 dB to -50 dB	< 0.1 dB or < 1°
	-50 dB to -65 dB	< 0.2 dB or < 2°
Specifications are based on a matched DUT, a measurement bandwidth of 10 Hz and a nominal source power of -10 dBm.		

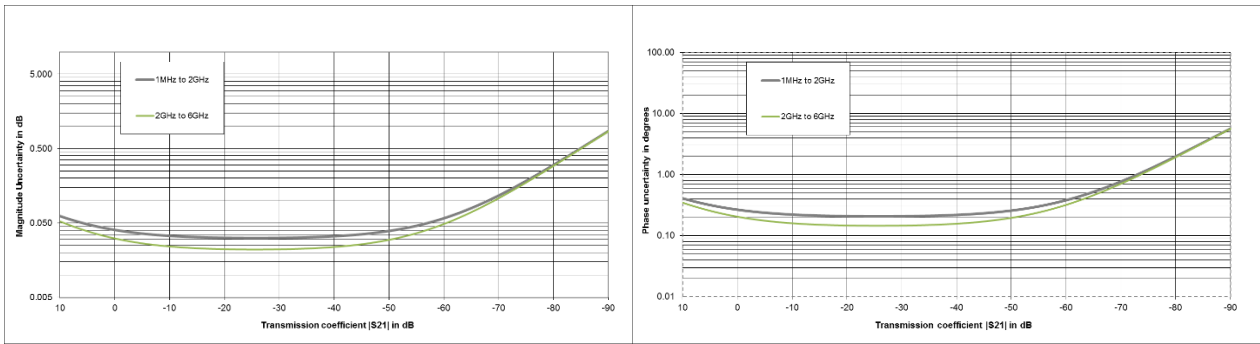

Typical accuracy of transmission magnitude and transmission phase measurements for the R&S®ZNLE<sup>1</sup>; analysis conditions:  $S_{11} = S_{22} = 0$ , calibrated power -10 dBm, measured power -10 dBm

Accuracy of reflection measurements	logarithmic			linear	
		magnitude	phase		magnitude
100 kHz to 6 GHz	0 dB	≤ 0.20 dB	≤ 1.3°	0 dB to -3 dB	0.024
	-3 dB	≤ 0.20 dB	≤ 1.3°	< -3 dB to -6 dB	0.016
	-6 dB	≤ 0.25 dB	≤ 1.5°	< -6 dB to -15 dB	0.013
	-15 dB	≤ 0.58 dB	≤ 4.0°	< -15 dB to -25 dB	0.012
	-25 dB	≤ 1.80 dB	≤ 13°	< -25 dB to -35 dB	0.012
	-35 dB	≤ 4.50 dB	≤ 42°		
Specifications are based on an isolating DUT, a measurement bandwidth of 10 Hz and a nominal source power of -10 dBm.					

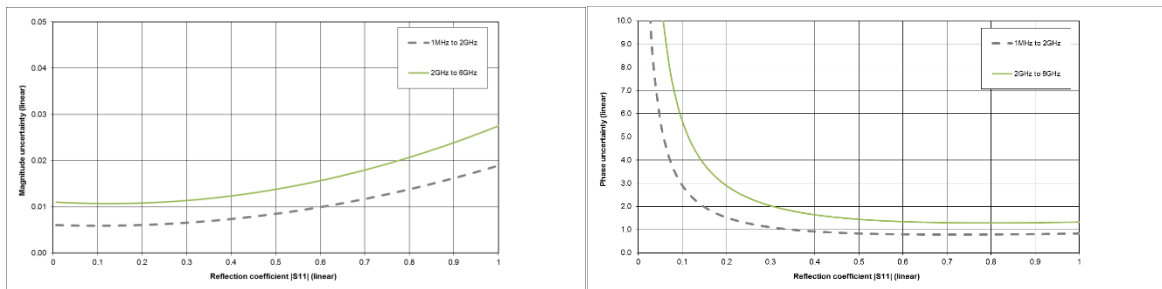

Typical accuracy of reflection magnitude and reflection phase measurements for the R&S®ZNLE<sup>1</sup>; analysis conditions:  $S_{12} = S_{21} = 0$ , calibrated power -10 dBm, measured power -10 dBm

## Effective system data



This data is valid between +18 °C and +28 °C, provided the temperature has not varied by more than 1 °C after calibration. Frequency points, measurement bandwidth and sweep time have to be identical for measurement and calibration (no interpolation allowed). The data is based on a measurement bandwidth of 10 Hz and system error calibration with an R&S®ZV-Z270 calibration kit using TOSM/SOLT with an R&S®ZV-Z270 calibration kit.

R&S®ZNLE <sup>1</sup>	100 kHz to 6 GHz
Directivity	≥ 40 dB
Source match	≥ 36 dB
Load match	≥ 40 dB
Reflection tracking	≤ 0.05 dB
Transmission tracking	≤ 0.05 dB

## Factory-calibrated system data

This data is valid between +18 °C and +28 °C. It is based on a source power of -10 dBm and a measurement bandwidth of 1 kHz.

		specification	typical
Directivity	100 kHz to 6 GHz	≥ 20 dB	30 dB
Source match	100 kHz to 6 GHz	≥ 20 dB	30 dB
Reflection tracking	100 kHz to 6 GHz	≤ 1.5 dB	0.5 dB
Transmission tracking	100 kHz to 6 GHz	≤ 1.5 dB	0.5 dB
Load match (raw test port match)	100 kHz to 3 GHz	≥ 14 dB	18 dB
Load match (raw test port match)	3 GHz to 6 GHz	≥ 12 dB	16 dB

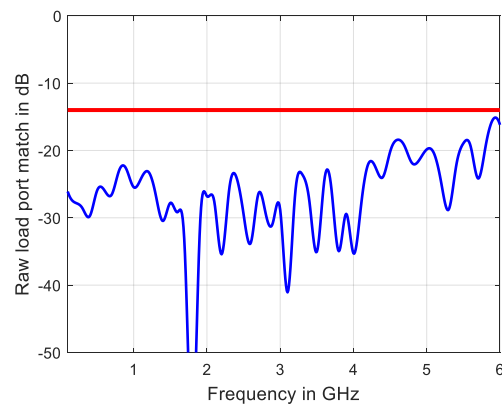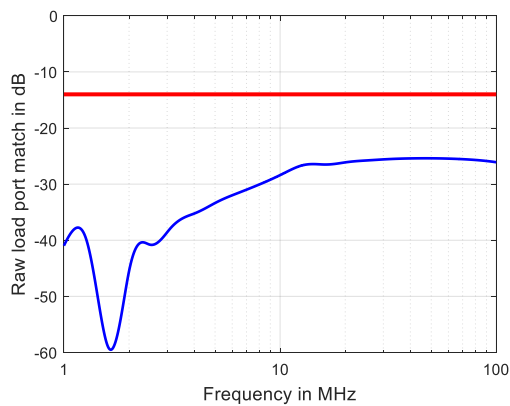



Raw load port match versus frequency for the R&S®ZNLE

Trace stability			specification	typical
Trace noise magnitude (RMS)	at 0 dBm source power, 0 dB reflection	IF bandwidth		
	100 kHz to 10 MHz	10 kHz	< 0.005 dB	0.001 dB
	10 MHz to 6 GHz	10 kHz	< 0.005 dB	0.001 dB
Trace noise phase (RMS)	at 0 dBm source power, 0 dB reflection	IF bandwidth		
	100 kHz to 10 MHz	10 kHz	< 0.1	
	10 MHz to 6 GHz	10 kHz	< 0.05	0.01°
Temperature dependence	at 0 dB transmission or reflection			
	100 kHz to 6 GHz	magnitude phase		0.05 dB/K 0.8°/K

## Test port output

This data is valid from +18 °C to +28 °C.

		<b>specification</b>	<b>typical</b>
Power range	100 kHz to 6 GHz	-10 dBm to 0 dBm	up to +2 dBm
Power accuracy, source power -10 dBm	100 kHz to 6 GHz	≤ 2 dB	0.5 dB
Power linearity referenced to -10 dBm		≤ 1.5 dB	
Power resolution		0.01 dB	
Harmonics source power -10 dBm	100 kHz to 6 GHz		-30 dBc

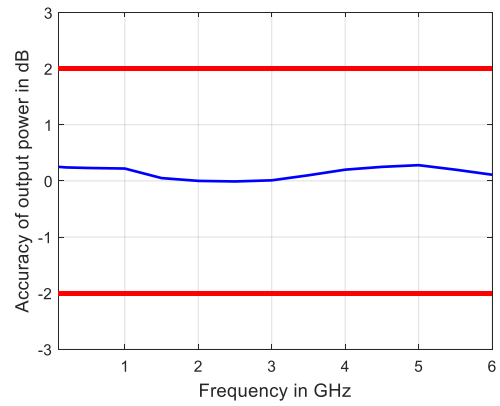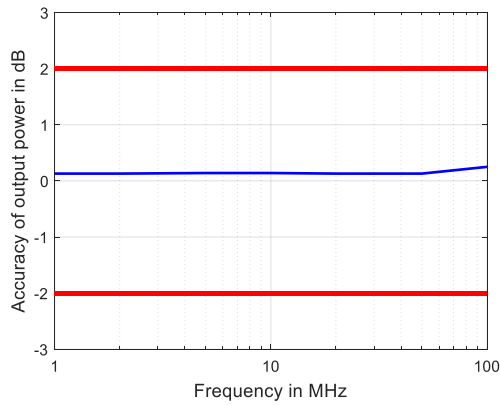



*Output power accuracy in dB versus frequency for the R&S®ZNLE base unit*



## Test port input

		specification	typical
Maximum nominal input level		0 dBm	
Power measurement accuracy	at -10 dBm without power calibration		
	100 kHz to 6 GHz	< 2 dB	0.3 dB
Receiver linearity referenced to -10 dBm	+10 dB to +5 dB	< 0.3 dB	0.2 dB
	+5 dB to -40 dB	< 0.2 dB	0.1 dB
Damage level		+27 dBm	
Damage DC voltage		30 V	
Noise level at 1 kHz measurement bandwidth, normalized to 1 Hz	100 kHz to 50 MHz	< -110 dBm (1 Hz)	-130 dBm (1 Hz)
	50 MHz to 6 GHz	< -120 dBm (1 Hz)	-130 dBm (1 Hz)

The noise level is defined as the RMS value of the specified noise floor.

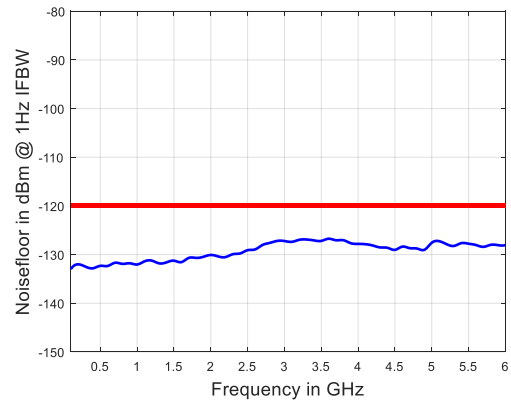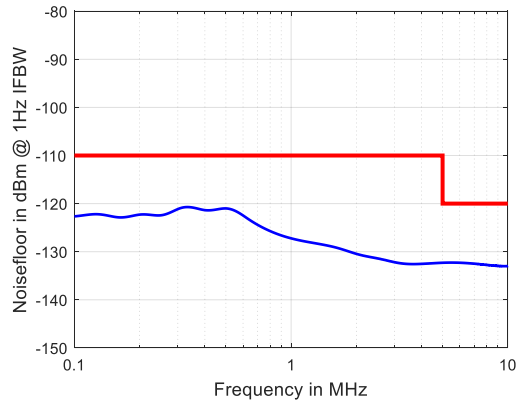

Noise level in dBm (1 Hz) versus frequency for the R&S<sup>®</sup>ZNLE

## Additional front panel connectors

USB	two universal serial bus connectors for connecting USB devices (USB 2.0); two additional USB 3.0 connectors on rear panel
-----	--

## Display

Screen	26.4 cm (10.1") diagonal WXGA color LCD with touchscreen
Resolution	1280 × 800 × 262144 (high color, 125 dpi)
Pixel failure rate	$< 1 \times 10^{-5}$

## Rear panel connectors

LAN	local area network connector, 10/100/1000BASE-T, 8-pin, RJ-45
-----	---

USB	(two) universal serial bus connectors for connecting USB devices (USB 3.0); two additional USB 2.0 connectors on front panel
-----	---

MONITOR	DVI-D connector (for external monitor)
---------	--

<b>REF IN</b>	input for external frequency reference signal	
Connector type		BNC, female
Input frequency		10 MHz
Maximum permissible deviation		1 kHz
Input power		-10 dBm to +15 dBm at 50 Ω
Input impedance		> 10 kΩ

<b>REF OUT</b>	output for external frequency reference signal	
Connector type		BNC, female
Output frequency		10 MHz
Output frequency accuracy		80 Hz
Output power		+6 dBm ± 4 dB at 50 Ω

<b>EXT TRIG IN</b>	trigger input for analyzer	
Connector type		BNC, female
TTL signal (edge-triggered or level-triggered)		3 V, 5 V tolerant
Polarity (selectable)		positive or negative
Minimum pulse width		1 μs
Input impedance		> 10 kΩ

## Options

For subsequently activated options, all data sheet parameters are typical values until a calibration is performed.

### R&S®FPL1-B10

<b>GPIB interface</b>	remote control interface in line with IEEE 488, IEC 60625; 24-pin
-----------------------	---


## General data

<b>Data storage</b>		
Internal	standard	solid-state drive 32 Gbyte (nom.)
External		supports USB-2.0-compatible memory devices
<b>Environmental conditions</b>		
Temperature	operating temperature range	+5 °C to +40 °C
	storage temperature range	-20 °C to +70 °C
Climatic loading	without condensation	+40 °C at 85 % rel. humidity, in line with EN 60068-2-30,
<b>Mechanical resistance</b>		
Vibration	sinusoidal	5 Hz to 55 Hz 0.15 mm constant amplitude (1.8 g at 55 Hz), 55 Hz to 150 Hz acceleration: 0.5 g constant, in line with EN 60068-2-6
	random	10 Hz to 300 Hz, acceleration 1.2 g (RMS), in line with EN 60068-2-64
Shock		40 g shock spectrum, in line with MIL-STD-810E method No. 516.4 procedure I, MIL-PRF-28800F
<b>EMC</b>		in line with EMC Directive 2014/30/EU including IEC/EN 61326-1 <sup>5, 6</sup> , IEC/EN 61326-2-1, CISPR 11/EN 55011 <sup>5</sup> , IEC/EN 61000-3-2, IEC/EN 61000-3-3
<b>Recommended calibration interval</b>		1 year
<b>Power supply</b>		
AC supply		100 V to 240 V ± 10 %, 50 Hz to 60 Hz ± 5 %, 400 Hz ± 5 % class of protection I, in line with VDE 411
Current consumption		1.7 A to 0.8 A
Power consumption		max. 170 W, 80 W (typ.)
Safety		in line with EN 61010-1, IEC 61010-1, UL 61010-1, CAN/CSA-C22.2 No. 61010-1
Test mark		CSA, CSA-NRTL
<b>Dimensions and weight</b>		
Dimensions	W × H × D	408 mm × 186 mm × 235 mm (16.06 in × 7.32 in × 9.25 in)
Net weight, nominal		6 kg (13.22 lb)


<sup>5</sup> Emission limits for class A equipment.

<sup>6</sup> Immunity test requirement for industrial environment (EN 61326 table 2).


## Dimensions (in mm)

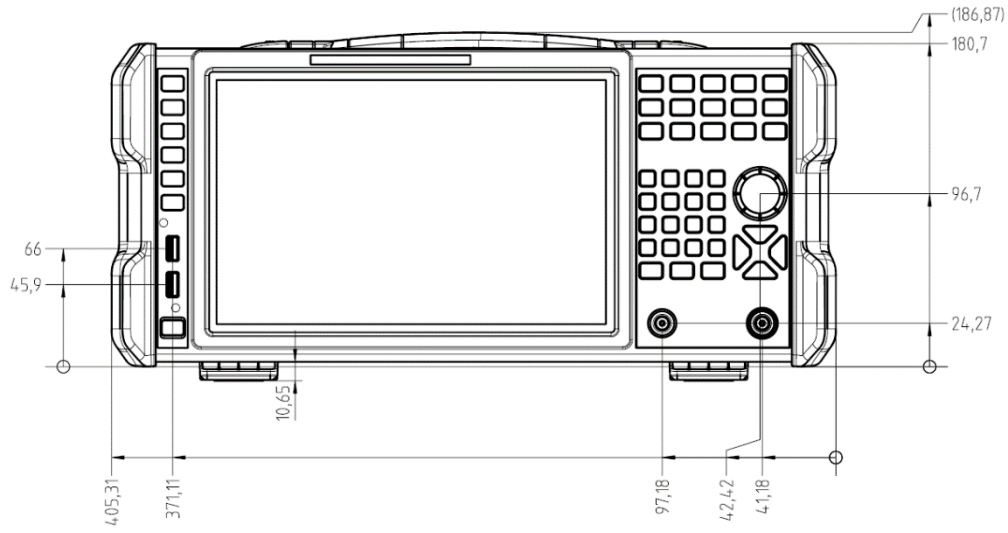

Front view

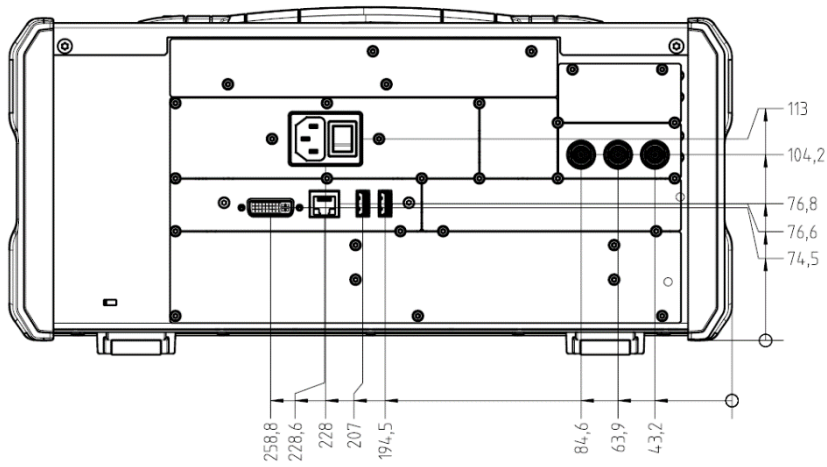

Rear view

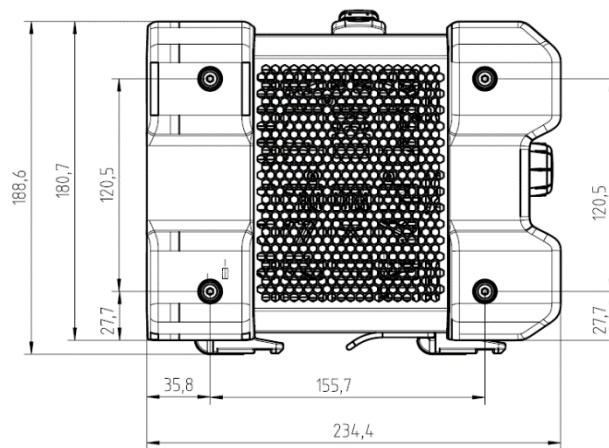

Side view

## Ordering information

Designation	Type	Retrofit <sup>7</sup>	On site <sup>8</sup>	Order No.
<b>Base unit</b>				
Vector network analyzer, two ports, 3 GHz, N	R&S <sup>®</sup> ZNLE3			1323.0012.53
Vector network analyzer, two ports, 4.5 GHz, N	R&S <sup>®</sup> ZNLE4			1323.0012.54
Vector network analyzer, two ports, 6 GHz, N	R&S <sup>®</sup> ZNLE6			1323.0012.56
<b>Options</b>				
Low frequency extension	R&S <sup>®</sup> ZNLE-B100	•	–	1303.9272.02
GPIB interface	R&S <sup>®</sup> FPL1-B10	•	•	1323.1890.02
<b>Firmware/software</b>				
Time domain analysis	R&S <sup>®</sup> ZNL-K2	•	•	1323.1819.02
Distance-to-fault measurement	R&S <sup>®</sup> ZNL-K3	•	•	1323.1825.02

<b>Warranty</b>				
Base unit			3 years	
All other items <sup>9</sup>			1 year	
<b>Options</b>				
Extended warranty, one year	R&S <sup>®</sup> WE1	Please contact your local Rohde & Schwarz sales office.		
Extended warranty, two years	R&S <sup>®</sup> WE2			
Extended warranty with calibration coverage, one year	R&S <sup>®</sup> CW1			
Extended warranty with calibration coverage, two years	R&S <sup>®</sup> CW2			
Extended warranty with accredited calibration coverage, one year	R&S <sup>®</sup> AW1			
Extended warranty with accredited calibration coverage, two years	R&S <sup>®</sup> AW2			

### Extended warranty with a term of one and two years (WE1 and WE2)

Repairs carried out during the contract term are free of charge <sup>10</sup>. Necessary calibration and adjustments carried out during repairs are also covered.

### Extended warranty with calibration coverage (CW1 and CW2)

Enhance your extended warranty by adding calibration coverage at a package price. This package ensures that your Rohde & Schwarz product is regularly calibrated, inspected and maintained during the term of the contract. It includes all repairs <sup>10</sup> and calibration at the recommended intervals as well as any calibration carried out during repairs or option upgrades.

### Extended warranty with accredited calibration (AW1 and AW2)

Enhance your extended warranty by adding accredited calibration coverage at a package price. This package ensures that your Rohde & Schwarz product is regularly calibrated under accreditation, inspected and maintained during the term of the contract. It includes all repairs <sup>10</sup> and accredited calibration at the recommended intervals as well as any accredited calibration carried out during repairs or option upgrades.

<sup>7</sup> Option may also be ordered at a later stage, upgrade in service.

<sup>8</sup> Option may be installed by the user on site.

<sup>9</sup> For options that are installed, the remaining base unit warranty applies if longer than 1 year.

<sup>10</sup> Excluding defects caused by incorrect operation or handling and force majeure. Wear-and-tear parts are not included.